


1/6

Fig. 1

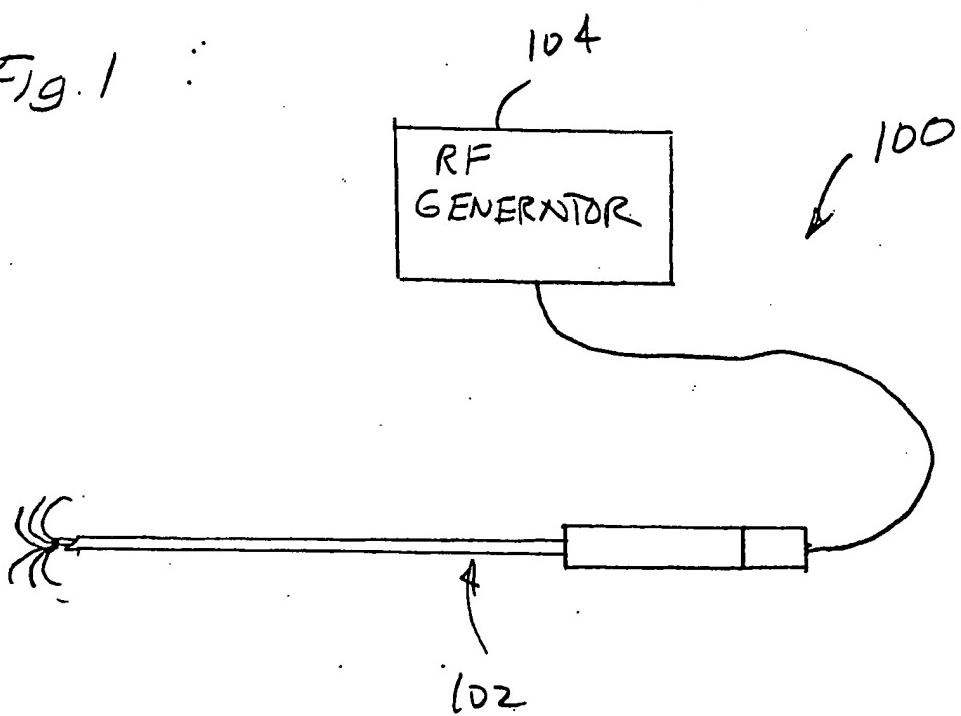

BEST AVAILABLE COPY

ABLATION PROBE WITH TEMPERATURE SENSITIVE ELECTRODE ARRAY

Robert J. Garabedian, et al

2024728-7034442001 (03-227)

Fig. 2

2/6



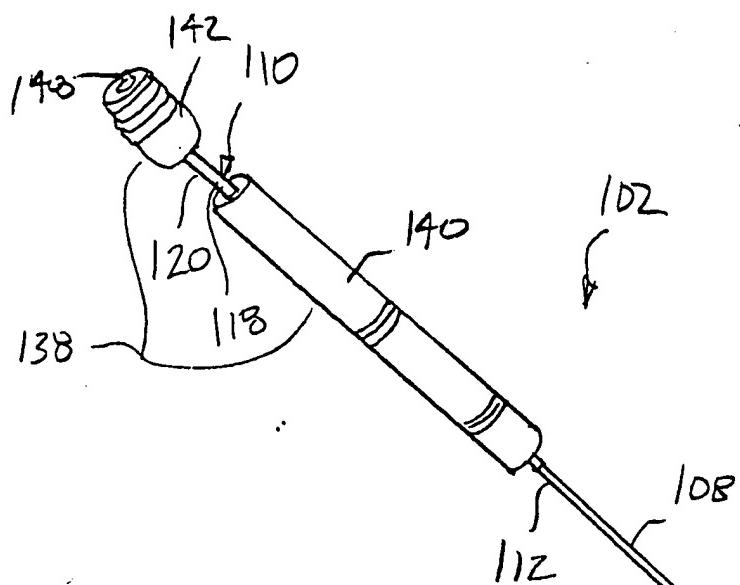


Fig. 3

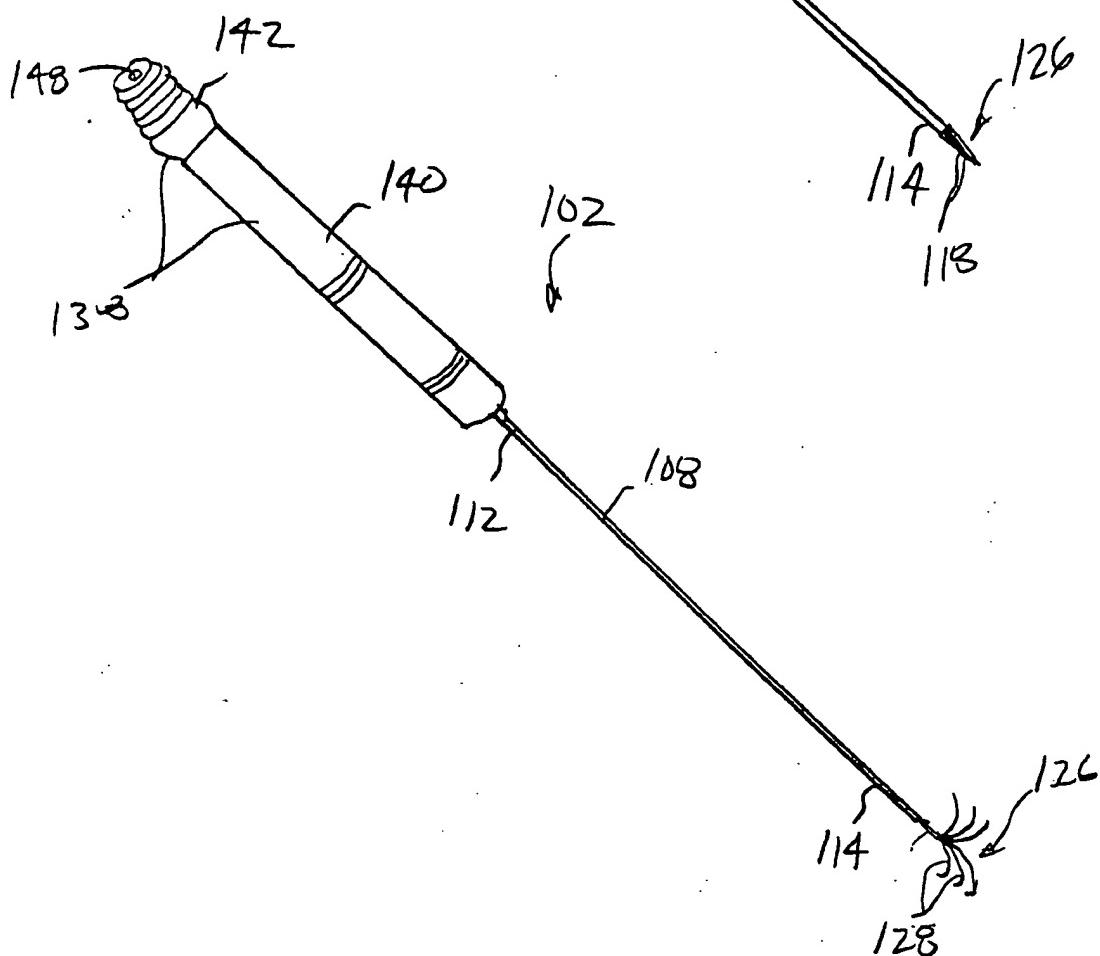

BEST AVAILABLE COPY

Fig. 4

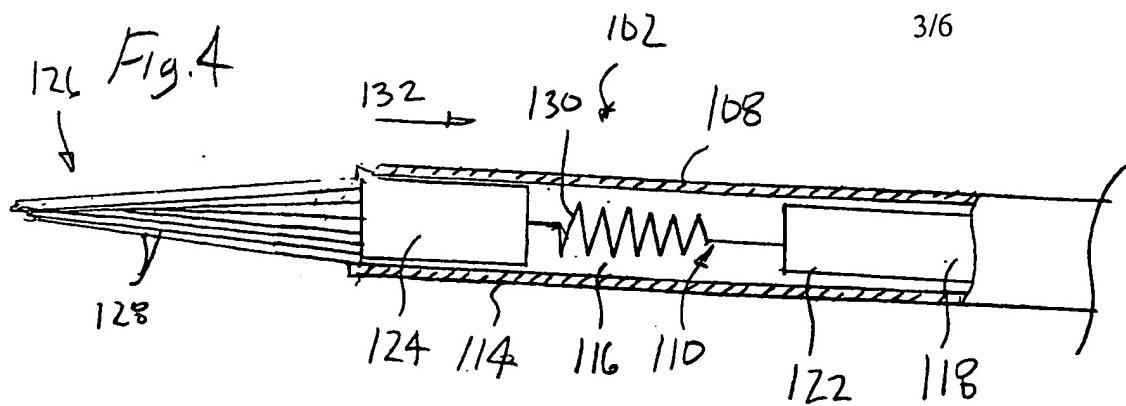

3/6

Fig. 5


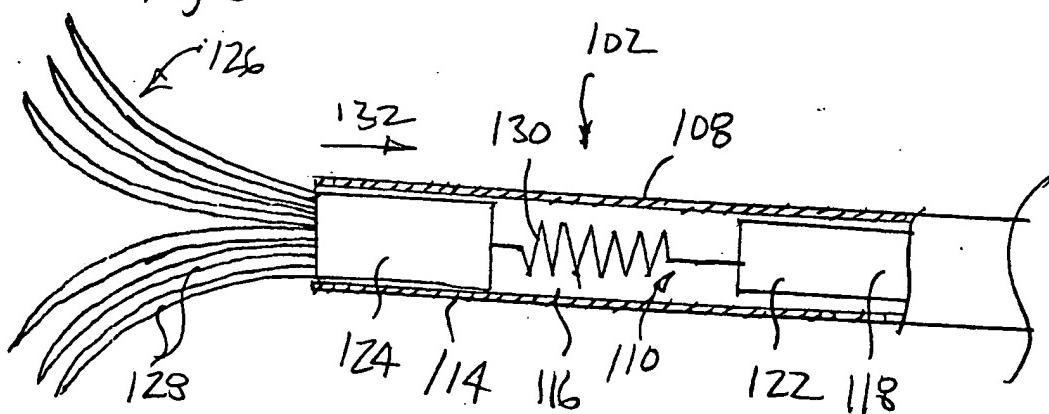


Fig. 6

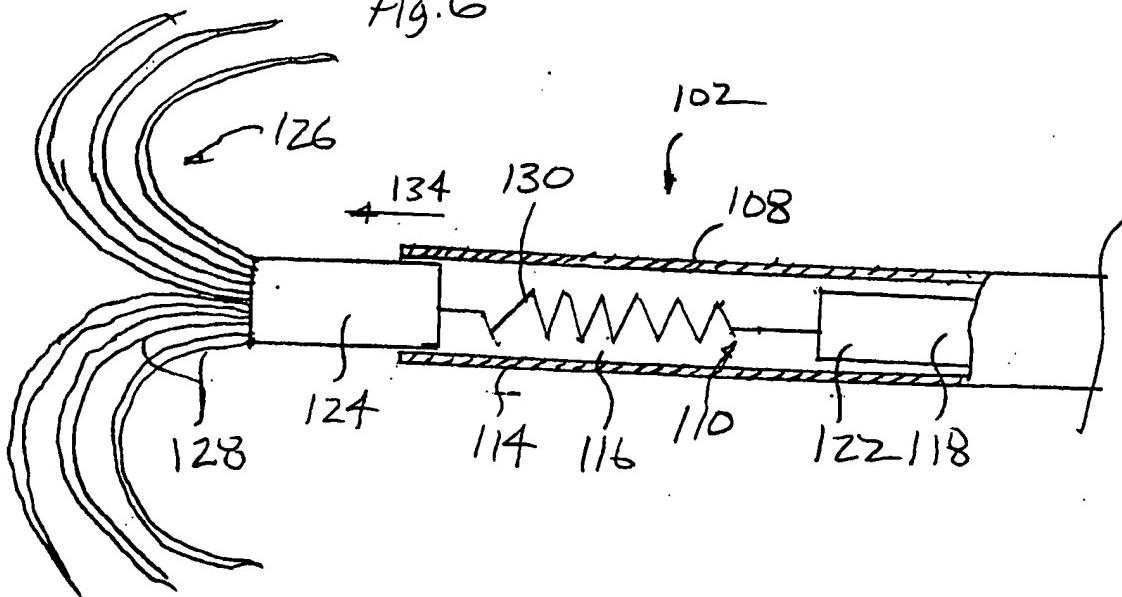

BEST AVAILABLE COPY

Fig. 7

4/6


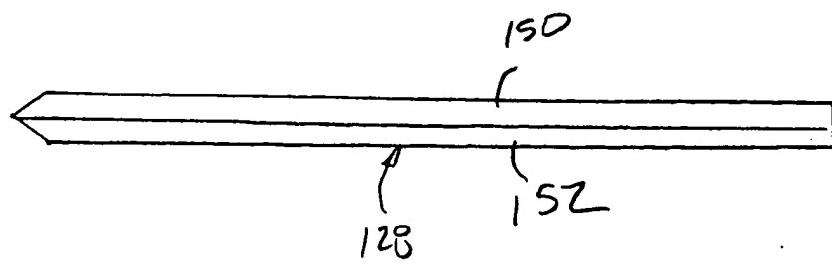


Fig. 8

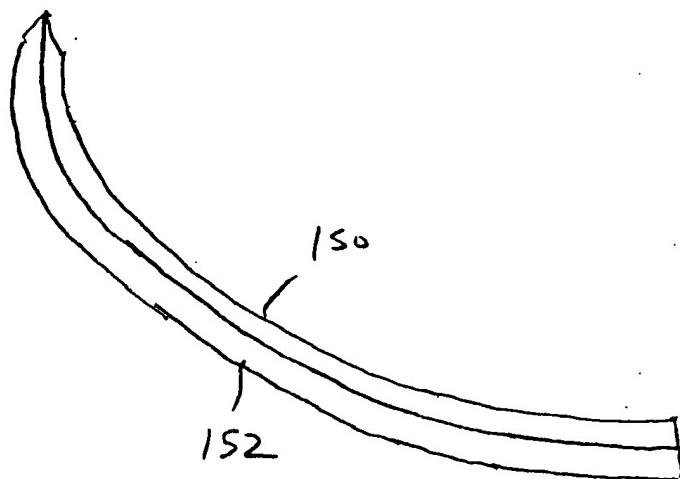

BEST AVAILABLE COPY

Fig. 9A

5/6


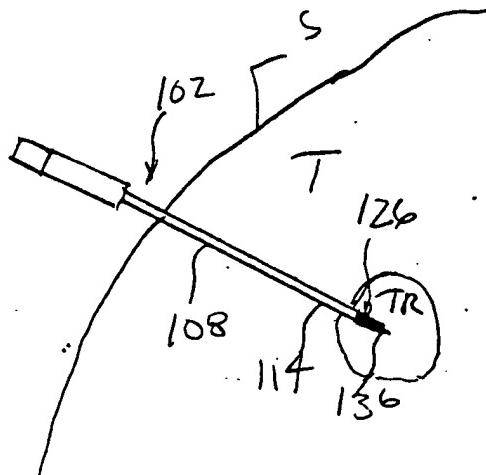


Fig. 9B

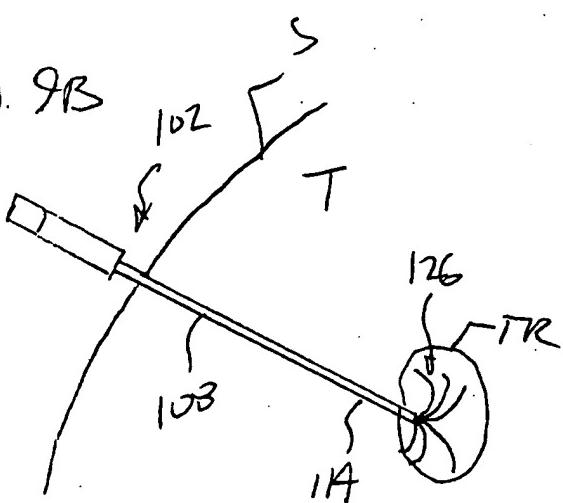


BEST AVAILABLE COPY

ABLATION PROBE WITH TEMPERATURE SENSITIVE ELECTRODE ARRAY
Robert J. Garabedian, et al
2024728-7034442001 (03-227)

6/6

Fig. 9C

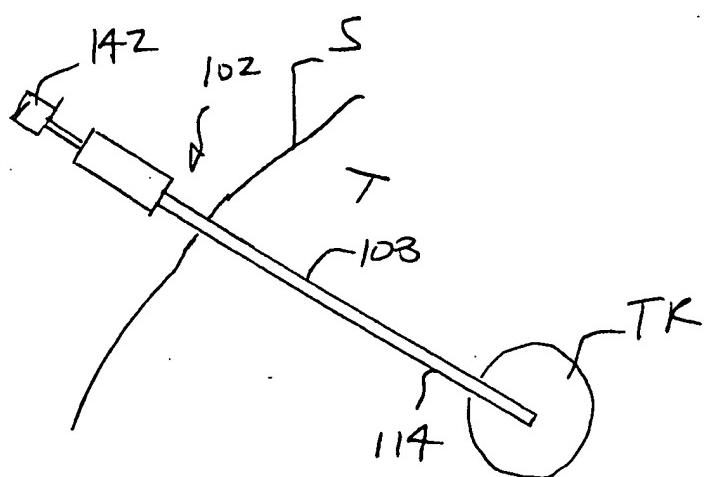

BEST AVAILABLE COPY